


## Achalasia Balloon Dilator

- total length 100 cm

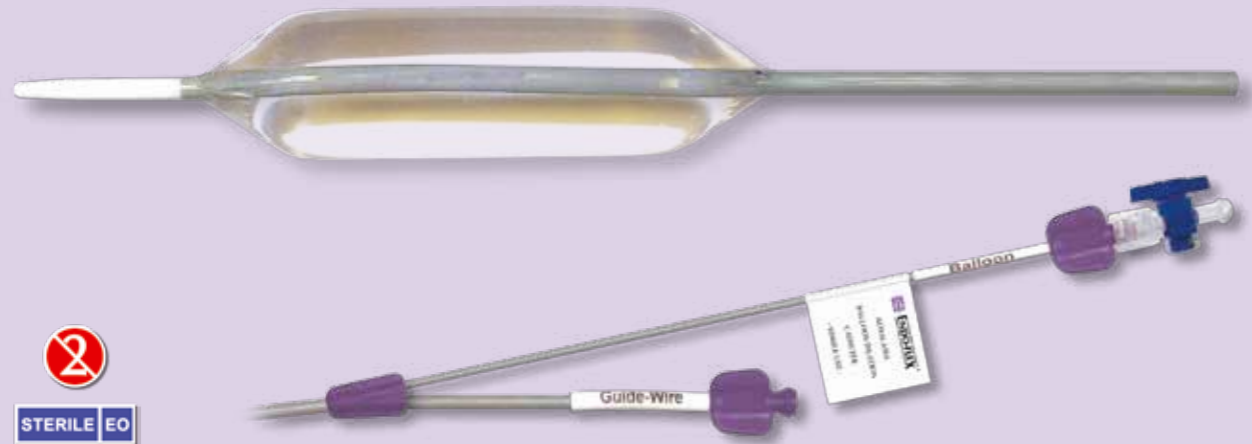


Order No.	Ø balloon	balloon length	fitting to working channel	Ø catheter	accepts guide wire
341 3080	30.0 mm	80.0 mm		4.7 mm	.035 inch
341 3580	35.0 mm	80.0 mm		4.7 mm	.035 inch
341 4080	40.0 mm	80.0 mm		4.7 mm	.035 inch

## recommended equipment

Inflation / Deflation Device incl. PSI-Manometer 0-440 PSI



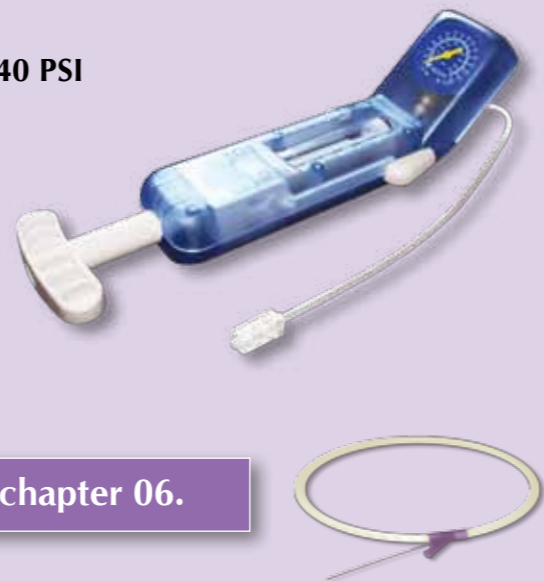

Order No. 340 800 INFL



Appropriate guide wires can be found in chapter 06.

### Legend:


-  This instrument is designed and warranted for single use only.
-  This instrument is sterile packed separately.

ENDO-FLEX GmbH  
 Alte Hünxer Str. 115  
 46562 Voerde / Germany  
 Phone: +49 281 - 9 44 00 - 0  
 Fax: +49 281 - 9 44 00 - 11  
 e-mail: export@endo-flex.de  
 www.endo-flex.de

© ENDO-FLEX - Technical specifications are subject to change


# DILATION BALLOONS

disposable

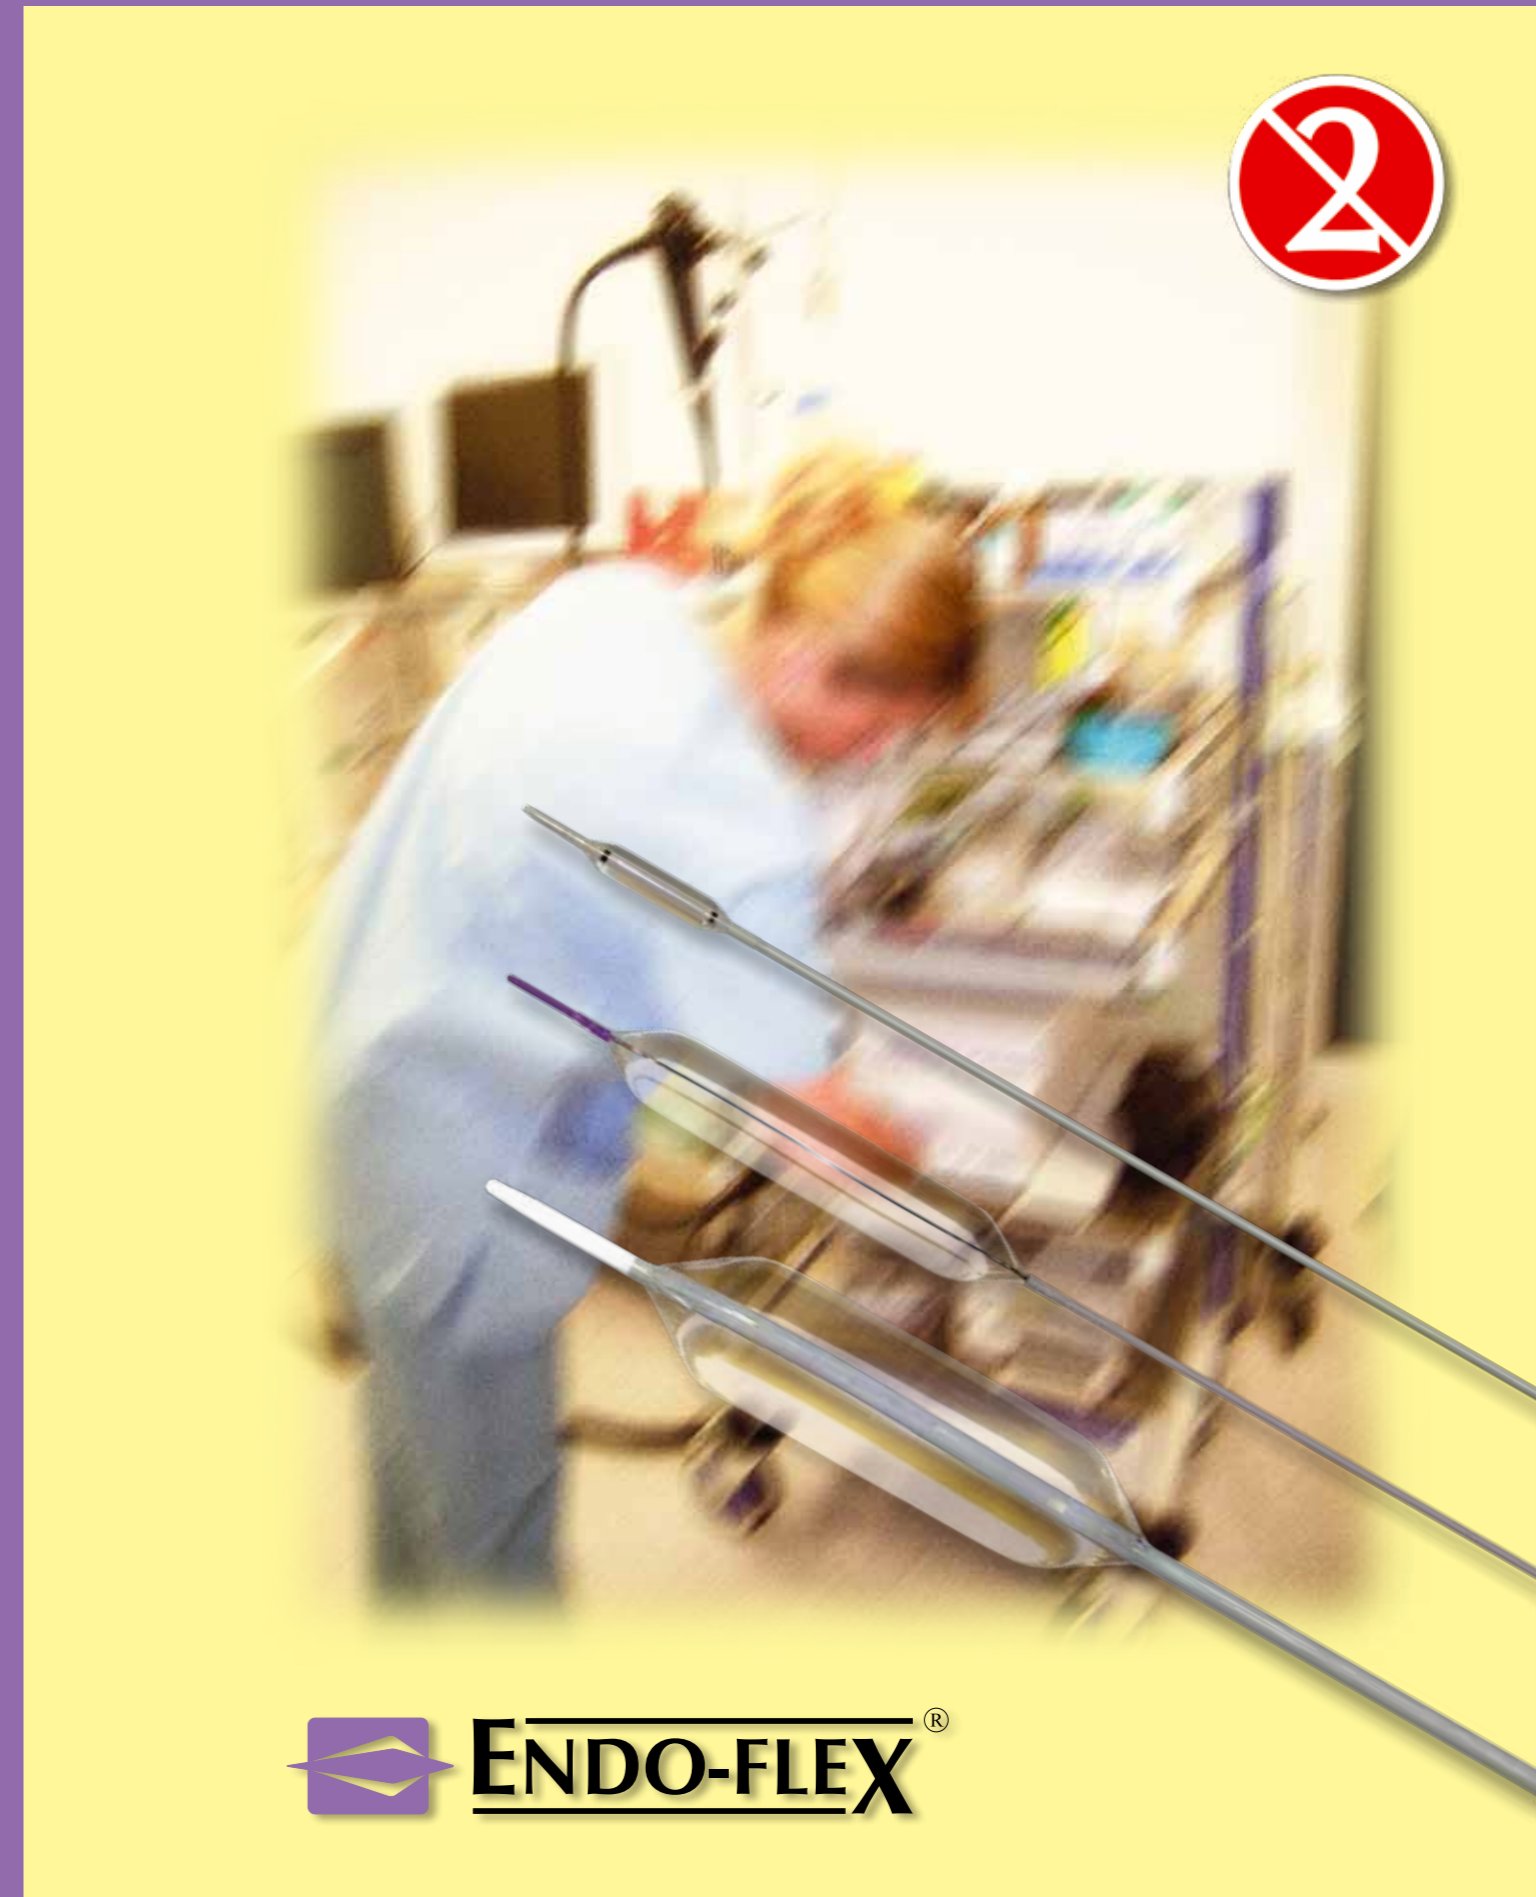

## Biliary Balloon Dilator

- total length 200 cm
- radiopaque markers

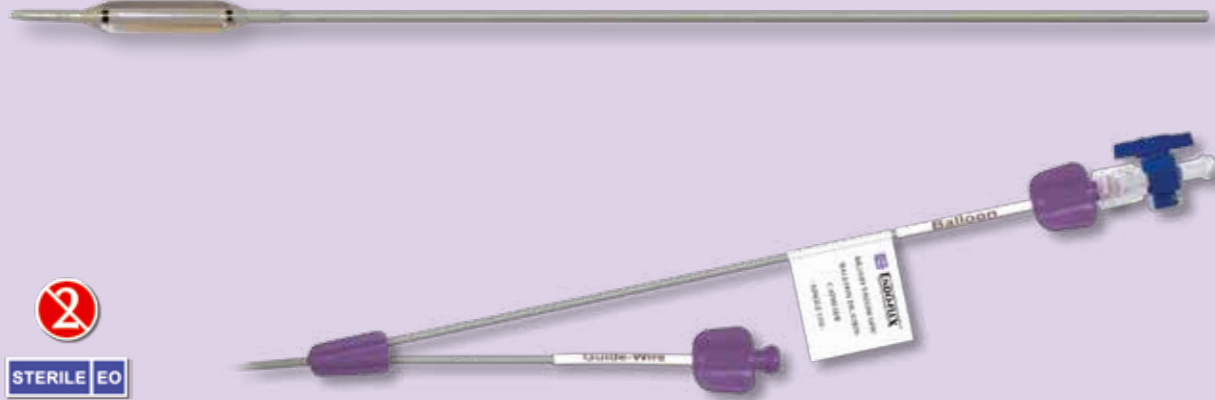

Order No.	Ø balloon	balloon length	fitting to working channel	Ø catheter	accepts guide wire
341 0420	4.0 mm	20.0 mm	2.8 mm	1.9 mm	.035 inch
341 0620	6.0 mm	20.0 mm	2.8 mm	1.9 mm	.035 inch
341 0830	8.0 mm	30.0 mm	2.8 mm	1.9 mm	.035 inch

### recommended equipment

Inflation / Deflation Device incl. PSI-Manometer 0-440 PSI



Order No. 340 800 INFL



Appropriate guide wires can be found in chapter 06.



## Esophageal Balloon Dilator

- total length 200 cm
- radiopaque markers



Order No.	Ø balloon	balloon length	fitting to working channel	Ø catheter	accepts guide wire
341 0880	8.0 mm	80.0 mm	2.8 mm	1.9 mm	.035 inch
341 1280	12.0 mm	80.0 mm	2.8 mm	1.9 mm	.035 inch
341 1680	16.0 mm	80.0 mm	3.2 mm	1.9 mm	.035 inch
341 1880	18.0 mm	80.0 mm	3.2 mm	1.9 mm	.035 inch
340 0880	8.0 mm	80.0 mm	2.8 mm	1.9 mm	
340 1280	12.0 mm	80.0 mm	2.8 mm	1.9 mm	
340 1680	16.0 mm	80.0 mm	3.2 mm	1.9 mm	
340 1880	18.0 mm	80.0 mm	3.2 mm	1.9 mm	

### recommended equipment

Inflation / Deflation Device incl. PSI-Manometer 0-440 PSI



Order No. 340 800 INFL



Appropriate guide wires can be found in chapter 06.

